



Contents lists available at ScienceDirect

Neuroscience and Biobehavioral Reviews

journal homepage: www.elsevier.com/locate/neubiorev



Review

Illuminating the developing brain: The past, present and future of functional near infrared spectroscopy

S. Lloyd-Fox^{a,*}, A. Blasi^b, C.E. Elwell^c

^a Centre for Brain and Cognitive Development, Birkbeck, University of London, Malet Street, Birkbeck WC1E 7HX, United Kingdom

^b Institute of Psychiatry, King's College London, Box P50, De Crespigny Park, London SE5 8AF, United Kingdom

^c Biomedical Optics Research Laboratory, Department of Medical Physics and Bioengineering, University College London, Gower Street, London WC1E 6BT, United Kingdom

ARTICLE INFO

Article history:

Received 8 April 2009

Received in revised form 15 July 2009

Accepted 16 July 2009

Keywords:

Near infrared spectroscopy (NIRS)

Optical imaging

Infant

Developmental neuroscience

Functional brain imaging

ABSTRACT

A decade has passed since near infrared spectroscopy (NIRS) was first applied to functional brain imaging in infants. As part of the team that published the first functional near infrared spectroscopy (fNIRS) infant study in 1998, we have continued to develop and refine both the technology and methods associated with these measurements. The increasing international interest that this technology is generating among neurodevelopmental researchers and the recent technical developments in biomedical optics have prompted us to compile this review of the challenges that have been overcome in this field, and the practicalities of performing fNIRS in infants. We highlight the increasingly diverse and ambitious studies that have been undertaken and review the technological and methodological advances that have been made in the study design, optical probe development, and interpretation and analyses of the haemodynamic response. A strong emphasis is placed on the potential of the technology and future prospects of fNIRS in the field of developmental neuroscience.

© 2009 Elsevier Ltd. All rights reserved.

Contents

1. Introduction	000
2. Near infrared spectroscopy: general principles and methods of measurement	000
2.1. Instrumentation	000
3. The development and use of fNIRS for infants	000
3.1. The number of channels, sources and detectors	000
3.2. The cortical area of interest	000
3.3. Hair	000
3.4. The fNIRS headgear and probe development at Birkbeck/UCL	000
4. Study design: considerations and effects	000
5. Methods: NIRS signal processing and analysis of the haemodynamic response	000
5.1. Processing the optical signal	000
5.2. Analyzing the haemodynamic response	000
6. Interpretation of fNIRS data	000
7. Coregistration	000
8. Concluding remarks	000
Acknowledgements	000
References	000

1. Introduction

A decade has passed since near infrared spectroscopy (NIRS) was first applied to functional brain imaging in infants. This review is offered in recognition of the work that has been achieved over the last 10 years and the progress that has been made in developing

* Corresponding author. Tel.: +44 207 631 6327; fax: +44 207 631 6587.
E-mail address: s.fox@bbk.ac.uk (S. Lloyd-Fox).

this technique for the investigation of developmental cognitive neuroscience. Further refinement and application of NIRS over the next 10 years will contribute significantly to the advancement of our understanding of the developing brain. We believe that functional NIRS provides an essential bridge between our current understanding of cortical activity in the developing brain and our knowledge of adult human brain function. Whilst there is now a multitude of behavioural research on infant development, the majority of which use looking time paradigms with preverbal infants, the number of developmental cognitive neuroscience studies still remain low. fNIRS will allow us to elucidate the connections between localized cortical activity and behavioural responses during early human development. Moreover, NIRS systems are inexpensive and portable, can accommodate a degree of movement from the infants enabling them to sit upright on a parent's lap, and essentially can measure spatially localized patterns of haemodynamic activity allowing comparisons with fMRI data of adult human brain function. fNIRS is ideally suited for infant research, as will be evidenced in the following review.

Neuronal activation originates in the neurons as electrical signals are passed between cells. During this activation the metabolic demand of neurons changes, provoking an increase in oxygen consumption, local cerebral blood flow (CBF) and oxygen delivery. A typical haemodynamic response (see Fig. 1) to cortical neuronal activation in adults shows an increase in blood flow leading to an increase in oxy-haemoglobin (HbO₂) and a (relatively smaller) decrease in deoxy-haemoglobin (HHb) as it is displaced

from the veins, leading to an increase in total-haemoglobin (HbT) (Villringer and Chance, 1997). Neuroimaging methods either detect the direct activation related to electrical activity of the brain (e.g. electroencephalography (EEG), magnetoencephalography (MEG)) or the consequent haemodynamic response (e.g. positron emission tomography (PET), functional magnetic resonance imaging (fMRI), functional near infrared spectroscopy (fNIRS)).

Many of these techniques, which are well established in adults, have limiting factors restricting or preventing their use in infants. PET requires the use of radioisotopes, whilst fMRI and MEG require the participant to remain very still, usually swaddled or restrained. There has been some infant research published using these techniques (i.e. Dehaene-Lambertz et al., 2002; Huotilainen et al., 2003; Imada et al., 2006; Tzourio-Mazoyer et al., 2002), however this work has generally been restricted to the study of sleeping, sedated or very young infants. For many years, the primary choice for functional imaging in awake infants has been EEG, a non-invasive technique with high temporal resolution but relatively poor spatial resolution. The advent of the new technology, fNIRS, was a welcome addition to a limited choice of neuroimaging methods suitable for use in infants.

The relative attributes of the functional neuroimaging techniques that have been and are currently used with infants are outlined in Fig. 2. EEG and fMRI bear the closest relation to fNIRS, the former uses a similar experimental setting, whilst the latter measures the same haemodynamic response. The major advantage

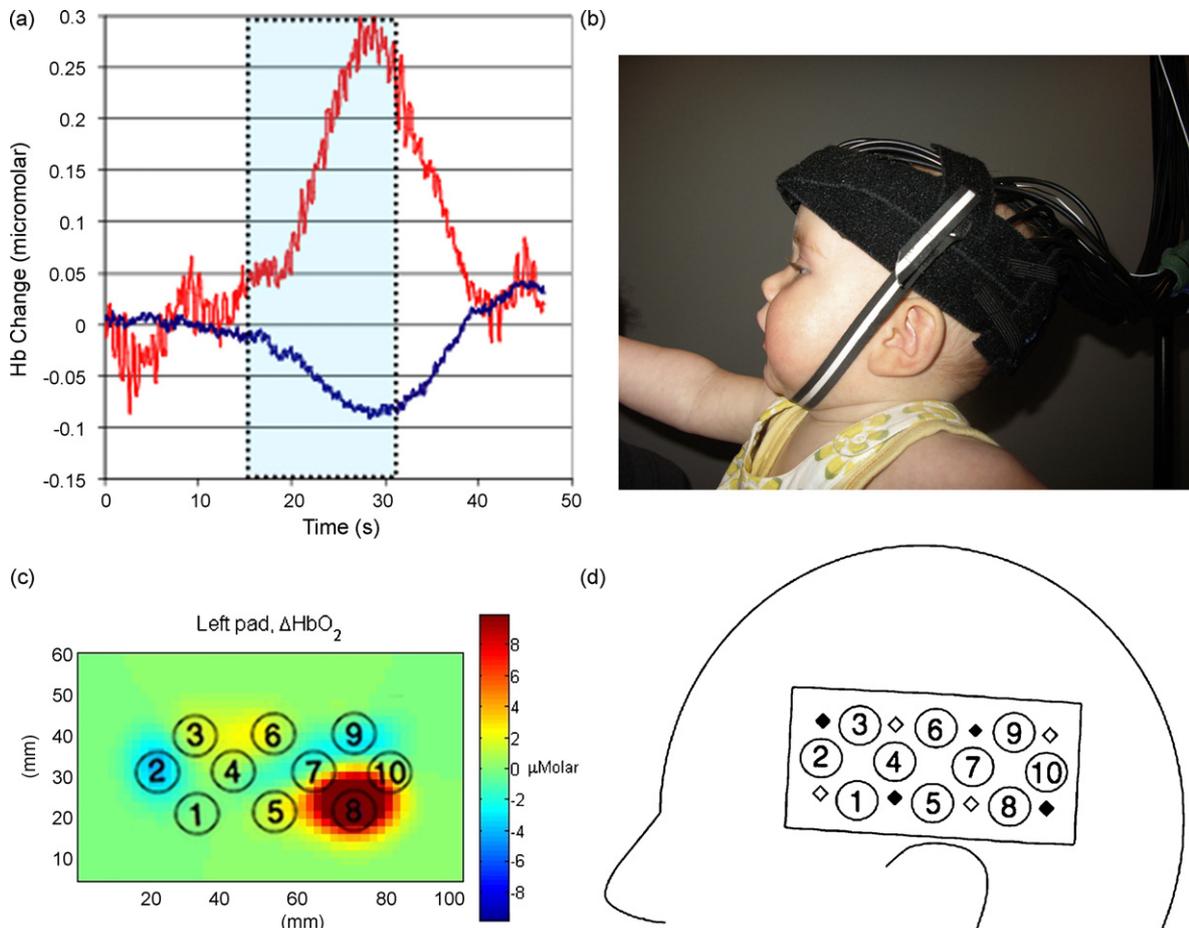


Fig. 1. An overview of the NIRS technique as applied to infants; (a) a typical haemodynamic response showing an increase in HbO₂ (red) and a decrease in HHb (blue) resulting from cortical activation (Courtesy of L. Coultts and A. Wilkins); (b) an infant wearing NIRS probes and headgear designed by the Birkbeck/UCL research team; (c) a linear reconstruction of changes in HbO₂ showing the spatial localization of the haemodynamic response to an experimental stimulus; and (d) the source-detector arrangement of the optical array used to collect the data shown in (c). (For interpretation of the references to color in this figure legend, the reader is referred to the web version of the article.)

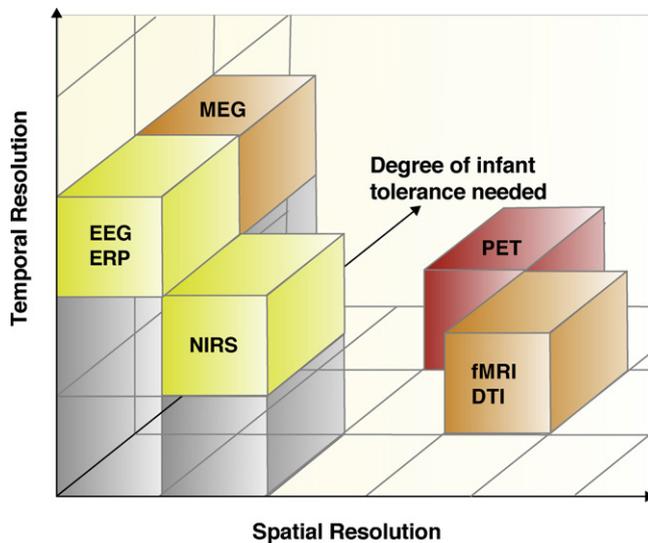


Fig. 2. This figure shows the spatial and temporal resolution of NIRS compared with other infant functional neuroimaging methods. It also illustrates the relative degree of tolerance needed from the infant for each method, ranging from yellow (low) to red (high). EEG, electroencephalography; ERP, event-related potential; MEG, magnetoencephalography; NIRS, near infrared spectroscopy; fMRI, functional magnetic resonance imaging; DTI, diffusion tensor imaging; PET, positron emission tomography. (This figure was inspired by Walsh and Cowey, 2000.) (For interpretation of the references to color in this figure legend, the reader is referred to the web version of the article.)

of fNIRS compared with EEG is that it is less susceptible to data corruption by movement artifacts and offers a more highly spatially resolved image of activation allowing the localization of brain responses to specific cortical regions. In addition, compared with fMRI, fNIRS has high temporal resolution, is silent allowing easy presentation of auditory stimuli, and can measure both oxy- and deoxy-haemoglobin chromophores (the molecules that are responsible for the colour of the blood due to their absorption of light at different wavelengths) providing a more complete measure of the haemodynamic response. Though fMRI and fNIRS measure the same haemodynamic response, generally fMRI techniques have an intrinsically limited acquisition rate usually at a minimum of one hertz (Huettel et al., 2003; but see Weishaupt et al., 2008), whereas fNIRS can acquire data rapidly, up to hundreds of hertz, thus providing a more complete temporal picture (Huppert et al., 2006). Naturally, as with any technique there are also limiting factors of NIRS; the temporal resolution is lower than EEG (the precision of which can reach up to a thousand hertz, Luck, 2005); the depth resolution is dependant on the age of the infant and the optical properties of the tissue (see Fukui et al., 2003); the technique offers lower spatial resolution compared with MRI; and there is no capacity for measuring brain structure for anatomical reference (see Minagawa-Kawai et al., 2008 for further discussion of these limitations). Despite these shortcomings a niche exists for fNIRS in developmental neuroimaging, which should be explored by more researchers. Moreover, research is underway to provide optimized measurements of brain activation by combining the advantages of several neuroimaging methods for the study of infants (see Section 7 for a further discussion). This practice has been successfully implemented in research with adult participants, e.g. combined fNIRS and EEG (Moosmann et al., 2003), fNIRS and MRI (Steinbrink et al., 2006) and fMRI and EEG (Dale and Halgren, 2001; Eichele et al., 2005). Aside from the advantages this presents for neurodevelopmental research, this multimodality approach has the potential to improve clinical neuromonitoring of preterm and term infants with acute brain injury (Toet and Lemmers, 2009).

The use of NIRS to study functional brain activation in infants is a rapidly increasing research area. Table 1a provides a summary of all of the infant fNIRS studies published over the last 10 years and demonstrates a fivefold increase in the number of papers published per year since 1998. This summary table illustrates how the study design, hypotheses, and cortical areas of interest have evolved and diversified. Whereas in the early fNIRS studies the main aim was to detect the response to basic stimuli activating the primary cortical areas such as acoustic tone in the auditory cortex (i.e. Sakatani et al., 1999) or stroboscopic flashing light in the visual cortex (i.e. Hoshi et al., 2000; Zaramella et al., 2001), more recently researchers have focused on more complex stimuli activating multiple cortical regions (see Table 1a). Moreover, an increasing number of researchers have focused on the study of awake infants to address topics such as; object processing (Wilcox et al., 2005, 2008; Watanabe et al., 2008), social communication (Grossmann et al., 2008; Minagawa-Kawai et al., 2009), biological motion processing (Lloyd-Fox et al., 2009), action observation (Shimada and Hiraki, 2006), and face processing (Blasi et al., 2007; Otsuka et al., 2007; Carlsson et al., 2008). In these studies, fNIRS has been used to localize haemodynamic responses in specific regions of the cortex such as the superior temporal sulcus (eye gaze/biological motion processing), orbitofrontal cortex (maternal face/emotion recognition), sensorimotor areas (action observation), prefrontal cortex (object permanence), and occipitotemporal cortex (dynamic objects) (see Table 1a). This capacity for localizing the cortical region of activation, and the allowance for movement of the participant, are the defining attributes of the application of the fNIRS method for the study of the early developing brain.

The ambition and drive to use fNIRS for increasingly complex studies continuously fuels the development of technologies and methods specifically for infant research. Practical issues that have arisen include; (1) the development of the probe and head gear to reduce the effects of movement of the infant, particularly important when studying visual paradigms where the infant is awake; (2) the design of the study, considering the effects of boredom, anticipation and the synchronization of systemic/biorhythmic responses; (3) an understanding of the haemodynamic response in infants and how to interpret a significant result; (4) and coregistration between the haemodynamic response measured at the surface of the head and the underlying cortical anatomy (for a review of these issues see Aslin and Mehler, 2005; Meek, 2002). Recent work in various research labs has led to major progress in these areas. For example, the development of multiple source-detector separation arrays to investigate depth discrimination of the haemodynamic response; an ever-increasing number of channels allowing for a wider coverage of the head; and advances in the design of the headgear providing improved quality of the optical signals. This review will consider these methodological and technological advances with particular focus on studies in awake infants. Importantly we will highlight the advantages of using NIRS for the study of infant development and outline prospects for the future.

2. Near infrared spectroscopy: general principles and methods of measurement

The use of near infrared light to monitor intact organs began as a discovery at a dinner table with the passage of light being observed through a steak bone at a family supper (Jöbsis vander-Vleit, 1999). Biological tissue is relatively transparent to light in the near infrared part of the spectrum allowing several centimetres of tissue to be illuminated. This fortuitous “optical window” coincides with the favourable differential absorption spectra of oxy- and deoxy-haemoglobin, thus allowing near infrared absorption spectroscopy methods to provide a non-invasive

Table 1a

An overview of the experimental setup, cortical regions of interest and findings of all infant functional NIRS studies published since the first study in 1998. A further two studies have been published in Chinese which are not included here; Hou et al. (2006a,b).

	First author	Year	Journal	Participants	Excluded infants	Cortical area of interest	Experimental stimuli	Exp. trial	Control stimuli	Con. trial	Significant results		
											HbO ₂	HbT	HHb
1	Meek	1998	Pediatr. Res.	20 infants (2–3 months)	38	Occipital and parietofrontal	VISUAL - checkerboard reversal	10 s	Blank dark screen	10 s	+	+	+
2	Sakatani	1999	Early Hum. Dev.	28 infants (neonates)	n/a	Frontal	AUDITORY - piano music	10 m	Silence	10 m	+	+	+(60%) –(32%)
3	Hoshi	2000	Pediatr. Neural.	7 infants (neonates) asleep	n/a	Occipital	VISUAL - stroboscopic light flash	30 s	Silence	1 m 30 s	++	+	+
4	Bartocci	2000	Pediatr. Res.	23 infants (neonates)	7	Orbitofrontal and olfactory	OLFACTORY own mother's colostrum, vanilla essence	30 s	Distilled water	2 m	+		
5	Zaramella	2001	Pediatr. Res.	19 infants (1–49 days) rest/sleep	n/a	Temporal	AUDITORY - tonal sweep of repeating sounds	2 m 40 s	Silence	4 m	+	+	+(62%)
6	Baird	2002	NeuroImage	12 infants (5–12 months)	n/a	Frontal	VISUAL object perm - toy hidden measure from point of occlusion	n/a	The previous visit when infant could not represent obj perm	n/a	+	+	↔
7	Pena	2003	PNAS	14 infants (neonates) asleep	2	Temporal	AUDITORY - mother's story, forward-FW or back-BW	15 s	Silence (S)	25–35 s		+	
8	Taga	2003b	PNAS	7 infants (2–4 months)	13	Frontal and occipital	VISUAL chequerboard (event relate)	3.2 s	Red and black schematic face 7–15 s + beep sounds	7–15 s	+		–
9	Taga	2003a	Early Hum. Dev.	25 infants (neonates) asleep	9	Frontal and occipital	VISUAL stroboscopic light flash	3 s	Silence	20 s	+		↔
10	Csibra	2004	J. Pediatr. Neural.	11 infants (4 months)	15	Frontal and occipital	VISUAL face/scrambled face	8 s	Cartoons (baseline calculated from 1 s prestim)	10 s	–	↔	+
11	Kusaka	2004	Hum. Brain Mapp.	5 infants (1–3 months) asleep	n/a	Occipital	VISUAL stroboscopic light flash	15 s	Silence	45 s	–	–(80%)	+
12	Kotilahti	2005	Neuroreport	20 infants (neonates) asleep	n/a	Temporal	AUDITORY 60 dB beeps sinusoidal	5 s	Silence	25 s	+		
13	Wilcox	2005	J. Biomed. Opt.	7 infants (6.5 months)	3	Temporal and occipital	VISUAL live - ball moving behind a	30 s	No visual or auditory stimuli	10 s	+	+	–Occip +Temp
14	Shimada	2006	NeuroImage	13 infants (6–7 months)	5	Temporal	VISUAL live vs. TV - exp. action with toy (AO) or invis action (OO)	20 s	Pendulum.	5 s	+		
15	Homae	2006	Neurosci. Res.	21 infants (3 months) asleep	10	Temporal	AUDITORY flattened and normal speech	4.1 s	Silence	12–15 s	+		
16	Homae	2007	Neurosci. Res.	21 infants (3 months) asleep	10	Temporal	AUDITORY flattened and normal speech	4.1 s	Silence	12–15 s	+		
17	Saito	2007a	Arch. Dis. Child.	20 infants (neonates) asleep	n/a	Frontal	AUDITORY speech, IDS or ADS (little red riding hood)	15–28 s	Computer generated white	1 m	+		
18	Blasi	2007	Phys. Med. Biol.	12 infants (4 months)	26	Occipital	VISUAL face v scrambled face	10 s	Cartoons	10 s	+		
19	Bortfeld	2007	NeuroImage	35 infants (6–9 months)	5	Temporal and occipital	VISUAL (V) ball and AUDIOVISUAL (AV) speech stimuli, 2 conditions	20 s	10 s baseline of blank screen silence	10 s	+		
20	Minagawa-Kawai	2007	J. Neurosci.	57 infants 4 age grps: 3–28 months	70	Temporal	AUDITORY pseudowords varied duration of vowel, 2 conditions	20 s	stimA continuously repeated instead of alternate	20 s			+
21	Otsuka	2007	NeuroImage	10 infants (5–8 months)	10	Temporal	VISUAL upright/inverted faces	5 s				+	+
22	Saito	2007b	Early Hum. Dev.	22 infants (neonates) asleep	n/a	Frontal	AUDITORY speech, emotive or monotone (little red riding hood)	30 s	Vegetable photos computer generated white noise	1 m	+		
23	Taga	2007	NeuroImage	15 infants (2–4 months)	30	Temporal	VISUAL chequerboard or AUDITORY voice (event rel)	3 s (V), 3 s (A)	Coloured shapes	12 s (V), 15 s (A)	+		–
24	Taga	2007	NeuroImage	9 infants (4–5 months) asleep	4	Temporal	AUDITORY speech sounds	3 s	Silence	12 s	+		–
25	Carlsson	2008	Acta Paediatr.	19 infants (6–9 months)	8	Frontal and occipital	VISUAL photos of mother and stranger face	15–20 s	Grey screen	15 s	+		↔

adult NIRS studies show HbO₂ and HHb responses related to BOLD fMRI signal changes, infant data reveals a less consistent pattern of activation (Baird et al., 2002; Hoshi et al., 2000; Meek et al., 1998; Sakatani et al., 1999; Wilcox et al., 2005; Zaramella et al., 2001) and simultaneous fNIRS/fMRI studies in infants would be a valuable addition to this field of research. These issues will be discussed further in Sections 6 and 7.

2.1. Instrumentation

Several techniques have been developed to measure the haemodynamic response using NIRS: continuous wave, time-resolved, spatially resolved and frequency-resolved spectroscopy (for review see Minagawa-Kawai et al., 2008; Wolf et al., 2007). The majority of fNIRS infant research has been undertaken using continuous wave (CW) systems (e.g. Blasi et al., 2007; Hintz et al., 2001; Peña et al., 2003) as they provide the simplest approach (for a detailed report see Hebden, 2003). Beyond standard commercialized systems there is an opportunity to measure with multiple wavelengths to enhance spectral resolution not just of the haemodynamic chromophores but also of cytochrome oxidase, a chromophore which may provide a marker of cellular oxygen metabolism (Heekeren et al., 1999). However, the CW-NIRS systems that have been used for functional activation studies in infants typically measure attenuation changes at only two wavelengths to provide changes in the concentration of the two chromophores HbO₂ and HHb (see Table 1b). The selection of these two wavelengths is an important issue and has been shown to affect the accuracy of the HbO₂ and HHb measurements. Several studies have suggested paired wavelengths of approximately 690 nm and 830 nm are optimal (Yamashita et al., 2001; Strang-

man et al., 2003; Boas et al., 2004; Sato et al., 2004). Uludag et al. (2004) determined that cross talk is reduced and separability is increased between the HbO₂ and HHb signals if one wavelength is below 720 nm and the other is above 730 nm. However it is important to note that these studies have used experimental data and theoretical models based on adult rather than infant head geometry. Further discussion of the influence of infant head geometry on the measured fNIRS signals is given in Section 3.

CW optical topography systems which use arrays of multiple sources and detectors (Fig. 1b and d) have been developed to provide two-dimensional maps of the cortical haemodynamic response (and therefore brain activity) (Blasi et al., 2007, Fig. 1c). Each detector records the amount of light coming from a subset of neighbouring sources, with each source-detector pair called a channel. To identify the source associated with a given detected signal either the sources are illuminated sequentially or are intensity modulated at unique frequencies. If using the latter method, the signals are then decoded in hardware using lock-in amplifiers or in software using a Fourier transform. In this way, measurements can be taken at a rate of several Hz, typically between 1 and 10 Hz, enabling the time course of the haemodynamic response to be accurately charted. As shown in Table 1b the majority of infant fNIRS studies have been performed using multi-channel optical topography systems.

In addition to CW-NIRS systems, time-resolved (TR-NIRS) and frequency-resolved (FR-NIRS) spectrometers can be used to derive absolute concentrations of oxy and deoxy-haemoglobin, although these techniques are generally impractical for infant fNIRS studies. However these systems may be of use in determining the spatial and temporal variations in optical pathlength which could influence the measured haemodynamic response (Ijichi et al., 2005; Sakatani et al., 2006).

Table 1b

An overview of the specifications of the NIRS systems used in the infant functional NIRS studies published since 1998.

	First author	Year	NIRS system	Wavelengths (nm)	Sources	Detectors	Channels	Chan Sep (mm)
1	Meek	1998	Hammamatsu NIRO 500	775, 825, 850, 905	1	1	1	35
2	Sakatani	1999	Hammamatsu NIRO 500	775, 825, 850, 905	1	1	1	40
3	Hoshi	2000	Shimadzu OMM-100	780, 805, 830	3	3	3	25
4	Bartocci	2000	Hammamatsu NIRO 300	775, 810, 850, 910	1	1	1	40
5	Zaramella	2001	Hammamatsu NIRO 300	775, 810, 850, 910	1	1	1	35
6	Baird	2002	Hammamatsu C546001	785, 830	1	4	4	20
7	Pena	2003	Hitachi ETG-100	780, 830	10	8	20	30
8	Taga	2003b	Hitachi NIROT	780, 830	10	8	12	20
9	Taga	2003a	Hitachi NIROT	780, 830	10	8	12	20
10	Csibra	2004	Hammamatsu NIRO 300	775, 810, 850, 910	2	2	2	40
11	Kusaka	2004	Shimadzu OMM-1080S	776, 804, 828	8	8	24	20
12	Kotilahti	2005	Helsinki (in house system)	760, 830	?	?	18	25
13	Wilcox	2005	Harvard (in house system)	690, 830	2	4	4	20
14	Shimada	2006	Shimadzu OMM-1080S	780, 805, 830	3	3	7	20
15	Homae	2006	Hitachi ETG-100	780, 830	20	16	48	20
16	Homae	2007	Hitachi ETG-100	780, 830	20	16	48	20
17	Saito	2007a	Hammamatsu NIRO-200	778, 812, 850	2	2	2	30
18	Blasi	2007	UCL NTS (in house system)	780, 830	8	8	30	14.3, 17.8, 22
19	Bortfeld	2007	Harvard (in house system)	680, 830	4	2	4	20
20	Minagawa-Kawai	2007	Hitachi ETG-100 and 7000	780, 830	2	2	4	30
21	Otsuka	2007	Hitachi ETG-100	780, 830	10	8	24	20
22	Saito	2007b	Hammamatsu NIRO-200	778, 812, 850	2	2	2	30
23	Taga	2007	Hitachi ETG-100	780, 830	10	8	24	20
24	Taga	2007	Hitachi ETG-100	780, 830	8	2	8	10, 20, 30, 40
25	Carlsson	2008	Hammamatsu NIRO-300	775, 810, 850, 910	2	2	2	40
26	Karen	2008	MCP-II (in house system)	730, 830	4	4	10	25, 37.5
27	Wilcox	2008	Harvard (in house system)	690, 830	2	4	4	20
28	Grossmann	2008	UCL NTS (in house system)	770, 850	11	12	27	20
29	Gervain	2008	Hitachi ETG-4000	695, 830	10	8	24	30
30	Watanabe	2008	Hitachi ETG-100 and 7000	780, 830	20	16	48	20
31	Nakato	2009	Hitachi ETG-100	780, 830	10	8	24	20
32	Nakano	2009	Hitachi ETG-100 (×2)	780, 830	20	16	48	20
33	Minagawa-Kawai	2009	Hitachi ETG-7000	780, 830	2	2	7	30
34	Wilcox	2009	Harvard (in house system)	690, 830	2	4	4	20
35	Lloyd-Fox	2009	UCL NTS (in house system)	770, 850	8	8	20	20
36	Bortfeld	2009	Harvard (in house system)	680, 830	2	4	4	20

3. The development and use of fNIRS for infants

fNIRS studies with infants can lead to high drop out rates compared with adults. The proportion of infants who cannot be included in a NIRS study due to unsatisfactory data is approximately 40% (measure obtained from the published papers described in Table 1a). This can be attributed, in a large proportion, to the difficulty of designing an efficient and comfortable method by which to attach multiple source and detector optodes to the infant head. Therefore, much time and many resources have been applied to their improvement to maximize the effectiveness of NIRS as a tool for infant research. The prerequisites for NIRS headgear for infant studies are that it must be comfortable, light-weight, easy to position in a very short space of time and must provide reliable continuous optical measurements from all channels. Unlike studies in adults, it is not possible to place the headgear on an infant, pause to assess the optical signals, adjust the position/fit of the headgear, and then begin the experiment. The headgear must fit securely on the head so that any movement of the infant does not alter the position of the source and detector fibres and lead to artifacts in the optical signal. The array of channels within the headgear must be contained within a semi-rigid structure allowing some flexibility to mold around the head while maintaining a fixed source–detector spacing across the array. The delicate optical fibres need to exit the head gear away from the infant's face and remain out of reach of their hands (see Fig. 1). During the positioning of the headgear the infants must not be unduly disturbed (this could lead to them being unwilling to start the study) and during the recording the headgear must be sufficiently unobtrusive to ensure that it does not distract the infants from focusing on the task.

A promising area for future fNIRS infant research is in the investigation of differences between individuals, which for example could help identify markers of typical and atypical processing in infants at risk of developing disorders such as autism and thus contribute to diagnosis and intervention programs. Sample sizes are typically small in clinical population studies of this kind and so it is particularly important that headgear design is optimized to provide robust optical data and to minimize the proportion of excluded data.

The last decade has witnessed an increasingly sophisticated array of designs for NIRS probes and headgear for infant studies, with important developments from a number of research labs including those at Harvard (Franceschini et al., 2006; Siegel et al., 1999) and the University of London (Blasi et al., 2007; Lloyd-Fox et al., 2009). Developments have also been made in a number of commercial NIRS systems such as the ETG Optical Topography system (The Hitachi Medical Corporation, <http://www.hitachimedical.com>) and the Imagent (ISS Inc., <http://www.iss.com>).

An overview of these recent developments in relation to some of the factors that influence probe and headgear design is discussed below.

3.1. The number of channels, sources and detectors

The development of optical topography has enabled researchers to increase coverage over the cortex, allowing comparisons of activation within and between broad areas such as frontal and temporal or occipital cortices. Whereas at first, fNIRS studies used a restricted number of channels (the first five published studies used only 1–3 channels, see Table 1b), this number has steadily increased and been incorporated into the design of the probes. A major limitation of restricting measurements to just one or two channels is the level of uncertainty that the measurements are being made over the relevant cortical region. As the underlying brain anatomy is not imaged with NIRS it is essential to account for

individual differences in brain structure by measuring the signal over a relatively wide area of the cortex. For example an array with one or two channels which produces unpredicted haemodynamic changes, may be attributable either to an unexpected functional response or misplacement of the optodes relative to the region of interest (see Section 6 for further discussion). It is therefore advisable to use optical topography with multiple channels wherever possible. Hitachi Medical Systems, has recently developed probes capable of providing between 48 and 128 measurement channels (ETG Optical Topography System, <http://www.hitachimedical.com>). A study by Watanabe et al. (2008) at the University of Tokyo used an 84-channel design to investigate the functional activation response across a wide area of brain regions to mobile objects and a black and white chequerboard in 3-month olds. The results revealed that whereas the occipital cortex responded to both types of stimuli, the occipitotemporal and prefrontal regions responded specifically to the mobile objects evidencing localized functional organization of the cortex at a young age.

The in-house UCL system is capable of measuring between 20 and 45 channels (Everdell et al., 2005). As well as enabling the comparison of activation across brain regions, a recent infant study from the research group at Birkbeck/UCL (Lloyd-Fox et al., 2009) highlighted the potential of fNIRS for the investigation of specific activation within a given brain region using multiple channels. An increase in HbO₂, was observed in response to dynamic social stimuli, and was localized to specific channels in a bilateral posterior area of the temporal cortex thought to be homologous to the superior temporal sulcus region.

The advantages of increasing the number of channels are clear. However this is confounded by the inevitable increase in weight and size of the headgear. This may explain the higher proportion of excluded optical data due to excessive movement artifacts in those fNIRS studies using a high number of channels. For example Watanabe et al. (2008) used up to 84 channels to measure multiple cortical regions but excluded data from almost 70% of the participants (see Table 1a). Similarly, Nakano et al. (2009) used a 48-channel system and excluded data from 56% of the participants. Given that the average proportion of excluded data for NIRS infant studies is around 40%, and can be as low as 12.5% (see Table 1a), these values are rather high. This is not to say that other studies where a lower number of channels were used have always reported a lower proportion of excluded data but rather that an increase in the number of channels is one factor that impacts the quality of the optical signal unless this is carefully considered within the headgear design.

3.2. The cortical area of interest

The cortical area of interest can affect the probe and headgear design in terms of the depth of the underlying cortex from the surface of the skin, the distribution and arrangement of the channels over the area of interest and the accommodation of the curvature of the skull.

Theoretically, if the source to detector distance is increased, the detected light is more likely to provide information about a haemodynamic response occurring in deeper tissue (Fukui et al., 2003). However, this assumption is limited by the intensity of the source light and the diffuse nature of optical scattering in tissue. To reach the cortex the separation between source and detector should be, at minimum, double that of the distance between the skin surface and the surface of the cortex. To ensure that the measurement is taken from within the cortex, when studying adult brain responses, the channel separations are usually between 40 and 50 mm (Okada et al., 1997). In infants, the skin, skull and CSF layer are all thinner and more translucent and so to reach the

cortex the channel separations are usually less (Fukui et al., 2003), between 20 and 30 mm (see Table 1b). The optimal separation for infants is a matter of much debate amongst NIRS researchers as there are several factors affecting this choice. An increase in the separation between source and detector will also lead to a decrease in the number of channels over a given area and will in turn affect the design of the headgear. Taga et al. (2007) investigated the optimal channel separation (between 10 and 40 mm) for recording the haemodynamic responses to auditory stimuli over the temporal lobes in 3-month-old infants and concluded that 20 mm provided the highest sensitivity to cortical activation. However it must be noted that the optimal separation may vary depending on the intensity of the source lights, the age of the infant and the area of the cortex under investigation. Firstly, the intensity of the light can effect measurements as the stronger the intensity, the more light will reach the detectors, and the better the signal to noise ratio will be in the optical signal. As the intensity of the sources can vary across NIRS systems, a separation that is ideal for one system may not be for another. Gervain et al. (2008) noted that an increase in the intensity of the light over two studies of auditory stimulation in infants had a causal relationship with the magnitude of the haemodynamic response. Secondly, over the first year of life the infant's brain and head rapidly increases in size causing the distances between anatomical layers to change over time, thus influencing the optimal channel separation. Thirdly, the anatomical structure of the head varies within and between individuals, for example in 5-month olds the cortex can be approximately 4 mm from the skin surface in the temporal lobe but at a greater depth of 10 mm in the frontal and occipital lobes (Salamon et al., 1990). Thus the optimal separation may vary across areas of the cortex and between individuals. In addition to using a single separation, one method to overcome the issue of choosing the ideal separation is to use a probe design that incorporates several source-detector separation distances. This multi-separation source-detector approach allows for several depths of the cortex to be measured simultaneously (see Blasi et al., 2007; Franceschini et al., 2007), leading to depth discrimination of cortical activation.

Finally, the curvature of the skull will have a dramatic effect on the design of the probe and headgear. As mentioned earlier, a major challenge is to ensure that the probe sits flat and securely against the head. Therefore, areas of the infant head that are more curved or have more individual variability, such as the forehead, are more difficult to accommodate. Despite these challenges, designs are now in use for occipital, frontal, temporal and parietal regional investigation.

3.3. Hair

Although the designs of the probes and headgear for fNIRS studies in infants have improved significantly there remains one issue that continues to frustrate researchers: the challenge of dealing with participants' hair. Firstly, hair reduces the grip of the headgear and probes on the head, lowering friction and increasing the effects of the movement of the infant. Secondly, the layering, differing orientation and colour of the hair lying between the probe and infant head will cause attenuation of the light and can lead to unreliable measurements. If the hair is particularly dark the optical data may simply be unusable. In adult studies, a great deal of time is spent moving hair away from the area directly under the optodes. This is largely impractical with infants as they will not tolerate much interference of the hair/headgear before becoming fussy. To combat the issue of hair in adults, designs such as the ETG system (Hitachi Medical Systems) spring-loaded optodes, capable of penetrating the hair layer, have been developed. However, the spring-loaded optodes are usually too uncomfortable for use with

unsedated infants. The effects of a moderate amount of hair can be overcome by ensuring the headgear is securely fitting, for example by using a chin strap and a silicon layer or similar gripping material on the probes to increase friction and prevent slippage of the headgear (the approach used in the most recent ETG system (Hitachi Medical) (Gervain et al., 2008) and the Birkbeck/UCL system (Lloyd-Fox et al., 2009)). In addition, by allowing a small space (a few mm) between the tip of the source/detector fibre and the scalp, the light will filter through the strands rather than being obstructed by a layer of flattened hair (as used in the Birkbeck/UCL system (Lloyd-Fox et al., 2009)).

3.4. The fNIRS headgear and probe development at Birkbeck/UCL

Our own work in this area has resulted from a multidisciplinary collaboration between the Centre for Brain and Cognitive Development (School of Psychology; Birkbeck, University of London) and the Department of Medical Physics and Bioengineering (University College London). As part of the team that published the first fNIRS infant study in 1998, we have steadily worked on developing and refining this technology. One of the priorities of the Birkbeck/UCL research group has been to develop probes and headgear to provide robust and reliable optical data over a high number of channels covering a relatively large area of the cortex. Whereas our first study using a high number of channels (30) (Blasi et al., 2007) resulted in the exclusion of 64% of the infant data, our most recent study (Lloyd-Fox et al., 2009) using 20 channels resulted in the exclusion of 20% of the data. The majority of the participants excluded in the most recent study were invalid because they did not attend to the stimulus for long enough and so we are confident that this reduction in data exclusion reflects the improvements in our headgear, which have made it more robust to head movement. As the design of the headgear has been a serious methodological issue for fNIRS users studying infants, there follows a brief outline of the improvements and practical adjustments that have been made to the design of the infant headgear by the Birkbeck/UCL research group.

- (i) *The optode holder* was changed from an end-on approach to, initially a prism-ended optode, and then a right-angled optode. This enabled the fibres to sit flush against the head and prevented them from pulling on the probes and headgear (see Fig. 3a). The prism-ended and right-angled optodes are also used by other NIRS systems (Benaron et al., 2000; Franceschini et al., 2007; Hitachi, <http://www.hitachimedical.com>).
- (ii) *A cloth headband* was designed to hold the fixed arrays of channels in the desired location on the head, with adjustable straps for different head sizes. This was a significant improvement compared with the Coban™ bandage (3M™ Coban™ self-adherent wrap; <http://solutions.3m.co.uk/>) used in the 2007 study (Blasi et al., 2007) as it reduced the degree of movement of the headgear relative to the head. The most recent headgear design incorporates a *second layer of headband* composed of a purpose made stretchy silicon band which is fastened around the head providing even pressure over the base of the probes while the cloth layer provides pressure over the top of the optodes (see Fig. 3b).
- (iii) In the design currently being used at the Birkbeck/UCL research lab the original plastic *optic fibres* have been replaced with *glass optic fibres* to improve flexibility, reduce the weight of the fibres pulling on the headgear and provide improved optical measurements. The latter benefit is achieved because light is absorbed less in glass compared with plastic fibres, thus improving the signal to noise ratio. This affect can be highly significant with at least one order of magnitude more

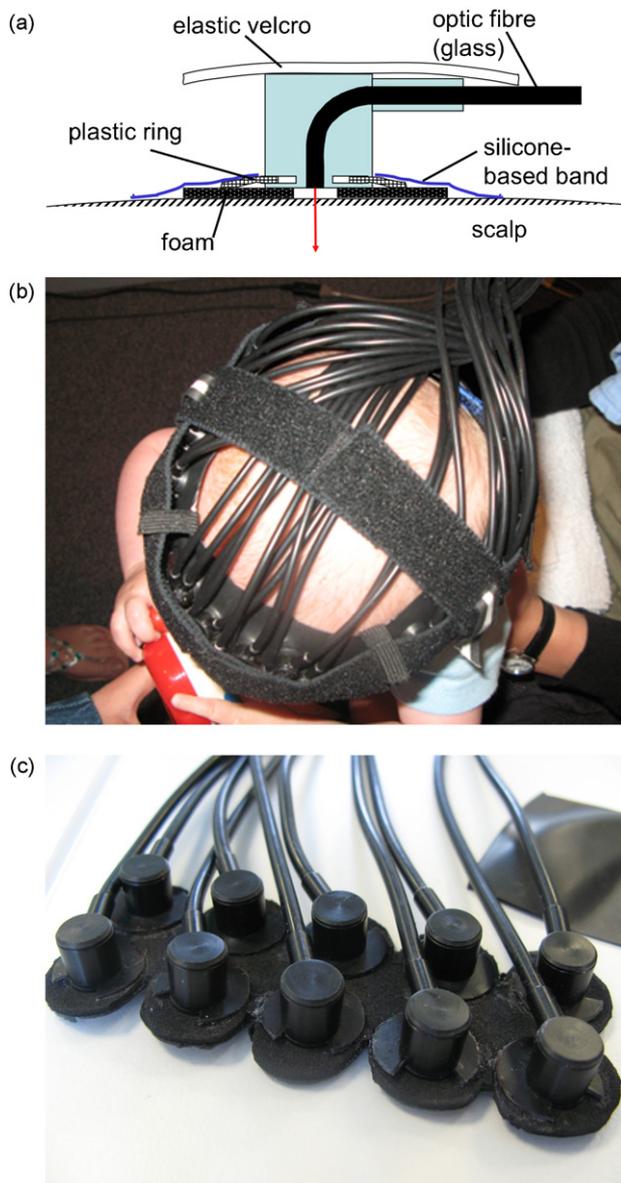


Fig. 3. A schematic of (a) the right-angled optodes; a photo (b) of an infant wearing the silicon and cloth layered headgear and a photo (c) of the glass optodes and fibres clipping into the probe. These were all designed at the Birkbeck/UCL research lab (figure (a) appears in Blasi et al., in press).

light transmitted through glass fibres than plastic fibres (unpublished observations).

- (iv) In recent work (Grossmann et al., 2008; Lloyd-Fox et al., 2009), the use of a *thin silicon layer* under the rigid array of optodes on the side in contact with the skin has increased the friction between the headgear and head and reduced slippage, which is particularly helpful when the infant has some hair. Silicon probes have also been used in the recent infant probes designed by Hitachi (i.e. Gervain et al., 2008).
- (v) The current design also offers *flexibility for channel arrangement and source-detector separation* as the glass fibres can clip in and out of the array to change the distribution of channels and the area of the cortex being investigated (see Fig. 3c). A similar technique is used by the team at Charité, University of Berlin (Boden et al., 2007).

At Birkbeck/UCL the combination of these modifications has improved the quality of the optical signal and enabled the

measurement of up to 45 channels covering the frontal and temporal regions of the brain. However it should be stressed that several of these modifications have also been devised concurrently at other research centres. These recent advances have enabled researchers to overcome some of the main challenges that fNIRS studies on the infant population have posed and have therefore further strengthened the role of NIRS as an important technology for studying infant cognitive development.

4. Study design: considerations and effects

First and foremost, the design of the study must take into consideration the temporal characteristics of the haemodynamic response (see Fig. 1a). With the exception of one study (Taga and Asakawa, 2007), the majority of infant NIRS work has been conducted using a block design for stimulus presentation. The common method is to present the experimental condition for a period of 3–30 s (or longer with auditory stimuli during sleep) followed by a control condition typically of longer duration to allow the haemodynamic response initiated during the experimental condition to return to a baseline level. This control condition is usually either of minimal stimulation (e.g. silence during sleeping studies) or designed to cause stimulation to a lesser extent than the experimental condition (e.g. use a mechanical movement in contrast to a biological movement in a region of the brain related to social perception as in Lloyd-Fox et al., 2009). Consequently the haemodynamic response to the experimental condition is measured in relation to the control condition.

An important consideration when designing a fNIRS study is the effect of physiological oscillations in the optical signal (e.g. vasomotion see Section 5). Further, it has been noted that infants are able to anticipate the onset of a stimulus (Csibra et al., 2001), which could in turn influence the onset of the haemodynamic response. One approach to reduce such physiological and anticipatory effects in a block design is to jitter experimental stimulus onset by varying the duration of the control trials so that they do not follow a predictable pattern. Alternatively, an event related design can also overcome these effects. A recent study by Taga and Asakawa (2007) used short stimulus presentations of 3.2 s for two types of experimental stimuli; auditory and visual. These stimuli were asynchronously presented with differing control trial durations to maintain unpredictable intervals of presentation. In this way, they were able to assess the effects of both types of stimuli relative to control, and found that only the auditory stimuli caused haemodynamic activation in the temporal lobe.

Finally, there are two considerations to be taken into account that affect the required number of trials for a given experimental condition. Firstly, one must establish the number of trial repetitions required for a robust response. Under ideal experimental conditions a single trial would be sufficient to yield a significant response (for an adult study see Colier et al., 1999; a study with awake infants see Carlsson et al., 2008; or studies with asleep infants see Saito et al., 2007a,b). However inadequate signal to noise and the presence of motion artifacts typically require the repetition of several trials. NIRS studies do not require as many repetitions as ERP studies where the proportion of excluded trials per experimental condition in infant studies can range from 30 to 50%. Secondly, the repetition of several trials can result in adaptation effects where neural responses to repeated stimuli can diminish over time (Krekelberg et al., 2006). In a recent infant fNIRS study by the Birkbeck/UCL research group of biological motion processing (Lloyd-Fox et al., 2009), the first five trials revealed a larger and more widespread pattern of activation than the analyses of all ten trials. If the signal to noise ratio is adequate fewer trials could yield more reliable data. It may therefore be

possible to design paradigms where relatively few trials are used to test multiple experimental conditions within one study.

5. Methods: NIRS signal processing and analysis of the haemodynamic response

The signal processing steps required to extract useable haemodynamic changes from the optical data typically involve (i) conditioning or smoothing the data by means of low-pass filtering and correction of linear trends (very slow fluctuations that could be of physiological origin); (ii) conversion of attenuation into changes in haemoglobin oxygenation (Beer-Lambert law, Kocsis et al., 2006); (iii) detection and removal of movement artifacts in the signal; and (iv) incorporation of an assessment of infant compliance/attention to the stimulus (typically extracted from the video recording of the session). In general these steps can be applied in any order since they all involve linear transformations. The analysis sequence used for the data collected in the Birkbeck/UCL studies is illustrated in Fig. 4. Steps (iii) and (iv) allow the selection of only the valid trials for block averaging and statistical analysis of the data. They ensure that the conclusions extracted from the study will be based on the true responses of the infants to the task assigned and not on spurious random effects from movement or other stimuli activating the same cortical region. Therefore it is important to have in place a set of objective criteria for this stage of the analyses. This and other issues involving the stages of NIRS signal processing and the techniques that are used at different research labs are discussed in detail below.

5.1. Processing the optical signal

Processing of the optical data usually starts with a channel by channel assessment of the quality of the data in order to immediately discard those channels affected by poor scalp coupling or instrumentation problems. All steps involved in the optical data processing summarised in Fig. 4, except the conversion from attenuation to haemoglobin oxygenation, are designed to eradicate the effects of various sources of noise in the data. There are three types of noise to consider when processing NIRS data: instrumentation, motion (from the infant), and physiological oscillations.

Signal noise originating from the instrumentation can be determined by performing NIRS studies on dynamic tissue mimicking phantoms (Koh et al., 2009) and can usually be removed using low pass filters.

Motion artifacts are usually characterized by abrupt changes in the signals occurring simultaneously in several channels—quite distinctive from the usual slow and smooth haemodynamic response. As previously discussed a secure design of the head gear can reduce the presence of such artifacts, although it is unlikely to completely solve the problem. One option to retrospectively deal with movement artifact is to use thresholding algorithms to remove sections of the data containing these abrupt changes (Lloyd-Fox et al., 2009; Peña et al., 2003). But thresholds must be defined carefully in order to preserve the changes that truly result from activation. There is no direct correlation between the type and strength of head movement and disruption of the optical data, therefore the use of a motion sensor to detect portions of the data affected by movement is not very effective. However, it is possible to use a motion sensor to evaluate the performance of infant head gear designs in terms of their robustness to movement and also to define thresholds for the automatic detection of artifacts (Blasi et al., in press). Other filtering techniques are available (see Matthews et al., 2008 for a review), for example the principal component analysis (PCA), as proposed by Wilcox et al. (2005), attempts to account for large movement artifacts across all measurement channels.

In contrast to movement artifacts, low frequency oscillations such as vasomotion (oscillations in vascular tone caused by local changes in smooth muscle constriction of the vascular wall unrelated to heart rate or respiration), can mimic in frequency and magnitude the haemodynamic response to stimulation (as demonstrated by Elwell et al., 1999; Katura et al., 2006; Taga et al., 2000). This can be overcome by careful design of the paradigm and the rate of stimulus presentation to minimise the possibility of coupling between functional activation and spontaneous cerebrovascular oscillations. In addition, in adults there is evidence of stimulus related changes in systemic parameters (e.g. heart rate, blood pressure, skin blood flow) (Obrig et al., 2000; Tachtsidis et al., 2008). Options for decoupling these systemic vascular changes and the cerebral haemodynamic response include the acquisition of systemic data by means of an independent measurement system, and the sampling of multiple volumes with NIRS so that measurements at the surface layer (with small source-detector separations) can be subtracted from measurements at the cortex level (larger source-detector separations) (Saager and Berger, 2008). Changes in systemic variables can also be accounted for using principal components analysis (PCA), by characterizing the systemic physiology features during the pre-stimulus control period and then removing the systemic

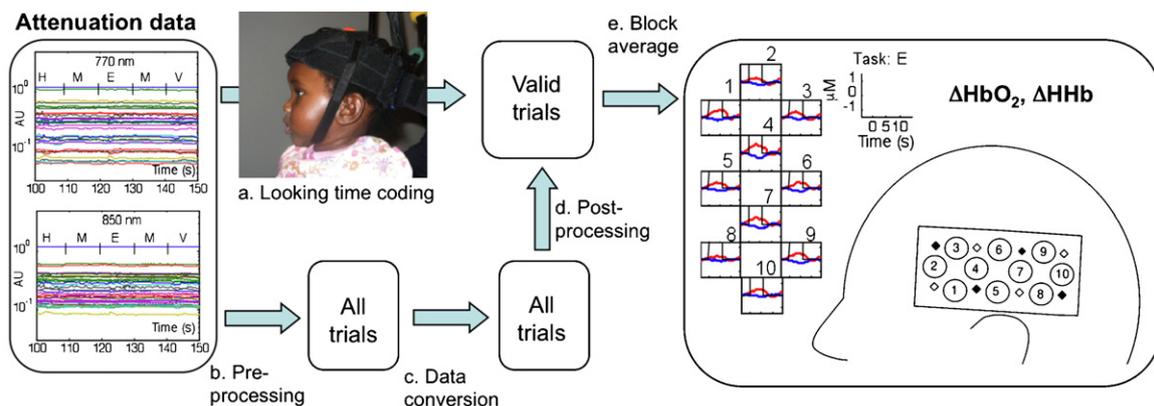


Fig. 4. Flow chart of the data analysis process as it is performed at the Birkbeck/UCL research lab. Infant looking time (a) is coded from a video recording of the session. Data pre-processing (b) involves low-pass filtering, channel by channel data quality assessment, construction of the trial blocks, and baseline correction within each trial block. The Beer-Lambert Law is used for the data conversion (c) from attenuation to haemoglobin oxygenation (HbO_2 , HHb) changes. Post-processing (d) consists in the automatic removal of movement artifacts. Finally, block averaging (e) and statistical analysis are carried out only in those channels that have good quality data (see Section 5.1 for a definition of a block) and within these, using only the trial blocks not affected by artifacts.

components in the experimental task period (Tachtsidis et al., 2008; Zhang et al., 2005).

Another important step in the data processing sequence is the removal of baseline trends across trials within the same session. Averaging the time courses of trials with different baselines could diminish the mean haemodynamic response. Baseline correction can be done by means of high-pass filtering or by simply removing a fitted line either across the whole study or within each block (a block is typically defined as including the period from the last few seconds of the control trial immediately preceding the experimental trial, the experimental trial, and the control trial that follows).

5.2. Analyzing the haemodynamic response

Traditionally, and due to the limited number of channels available in the first fNIRS systems, analysis of NIRS data has been based on time series processing, with standard *t*-tests to evaluate the significance of stimulus-correlated changes in the signals, or repeated measures analysis of the variance (ANOVA) to compare the shape (in time) of the response to different stimuli and/or groups of participants. With the incorporation of higher density arrays of sources and detectors, corrections for spatial correlation between closely placed measurement points have also been incorporated (Singh and Dan, 2006). Moreover, simultaneous acquisition of data from these multiple channel arrays has enhanced the potential of NIRS by opening the field to data reconstruction of functional images (Gibson et al., 2005). Indeed, the similarities between fMRI and optical experimental designs are being exploited and analysis techniques usually applied to fMRI are being adapted to optical data such as statistical parametric mapping techniques based on the general linear model (GLM) (Koh et al., 2007; Ye et al., 2009).

Being a relatively novel technique, it has been common practice for different groups using NIRS to develop their own analysis procedures and software. As an increasing number of research groups use optical topography for a wide range of functional studies that differ in their degree of complexity, age range, cortical region of interest, optode geometries and system configurations, it is paramount that we adopt a standard and robust analysis methodology (Schroeter et al., 2004). Several freeware packages are available for the analysis of optical signals each with the flexibility to accommodate different system configurations (HomER, Huppert et al., 2009; fOSA, Koh et al., 2007; NIRS-SPM, Ye et al., 2009), however some unification and standardization of data analysis methodologies may be beneficial to this research community.

6. Interpretation of fNIRS data

fNIRS measures the quantitative regional haemodynamic change that results from a localized change in brain activation state relative to a control state. As described earlier, an increase in HbO₂ and a decrease in HHb concentration represent the standard adult haemodynamic change, however from the very first fNIRS infant study in 1998, it was proposed that there could be a different infant-specific pattern of haemodynamic response. Despite numerous publications since then, controversy still remains regarding the exact nature of this infant response. Tables 1a and 1c summarizes the analysis methodologies used in the fNIRS infant publications and the resulting magnitude and directional changes seen in HbO₂ and HHb. HbO₂ and HbT changes related to cortical activation are highly consistent across studies and in general similar to that observed in adults. However, HHb results are far less consistent in infants, and consequently are often not reported in publications. In addition, individual infants and certain study

paradigms have shown unpredicted decreases in HbO₂. The situation is further confused when authors do not report results for both HbO₂ and HHb changes (44% of the published infant studies listed in Table 1a–c do not report both).

The majority of fNIRS infant studies (94% of the published infant studies listed in Table 1c use HbO₂ as the preferred measure for cortical activation. This is probably because this chromophore typically has the highest signal to noise ratio (SNR). Additionally, the direction of the HbO₂ change is the most consistent in infants and similar to that of adults: out of the 94% that reported HbO₂ changes, an increase in HbO₂ was reported in 93% of the studies. Controversially, the remaining 7% of the studies describing HbO₂ change, reported a consistent decrease in HbO₂ in response to the experimental stimuli. In a study by Csibra et al. (2004), a strong decrease in HbO₂ was recorded from a single channel positioned over the occipital cortex. In this case a decrease in HbO₂ could be related to an unpredicted increase in activation in response to the animated cartoons (control condition) relative to the static face stimuli (experimental condition) so that the baseline correction causes the appearance of 'deactivation' during the experimental condition. Alternatively, the single recording channel may have not been positioned over the optimal cortical region for face processing, an issue which reinforces the importance of multiple channel arrays that can investigate wider cortical regions. In a study by Kusaka et al. (2004) a significant decrease in HbO₂ was reported in response to stroboscopic flashing lights projected over the eyelids of sleeping infants. Further, a newborn study with the same paradigm using three channels over the occipital cortex found that only one of these three channels showed a significant increase in HbO₂ whilst the other two showed significant decreases (Hoshi et al., 2000). Relatively little is known about cortical activation during sleep, the sleeping state could induce neural inhibition in the visual cortex. In addition as these were infants of just 1–3 months of age, the haemodynamic properties of cortical activation may change over the course of development—this is discussed in detail later in this section.

As an increase in HbO₂ with no significant HHb change, would not represent activation in a BOLD contrast study (Obrig and Villringer, 2003) it is interesting to note that only 59% of the published infant studies (cited in Table 1c) report significant changes in HHb in addition to changes in HbO₂. Moreover, the direction of the HHb haemodynamic change is not consistent across the studies. Only 25% of these studies reported a decrease in HHb, whereas 40% reported an HHb increase. In the remaining 35% the changes were not consistent enough to draw conclusions or did not reach statistical significance. It has been suggested that ambiguity in the measured HHb change in adult data could be due to the choice of wavelengths used as discussed in Section 2.1 (Boas et al., 2004), but clearly an explanation based on physiology should also be sought, especially since the balance of oxygen supply and demand may differ in infants compared with adults. The haemodynamic response measured by fNIRS depends upon the combined effects of activation related increases in oxygen consumption (producing an increase in HHb and decrease in HbO₂) and oxygen delivery (producing an increase in CBF characterized by a decrease in HHb and an increase in HbO₂). The balance of these mechanisms determines whether there will be an increase or a decrease in HHb/HbO₂ concentration. In adults, typically the increase in CBF exceeds the demand for oxygen (Obrig and Villringer, 2003; Raichle, 1998) leading to an fNIRS measured haemodynamic response as shown in Fig. 1. However, in infants HHb/HbO₂ concentration changes related to neural activation do not follow a typical pattern as evidenced in Table 1c and may depend on age, the region studied, and sleep and/or sedation state, among other factors (Martin et al., 1999; Marcar et al., 2004, 2006; Meek, 2002; Wilcox et al., 2008). fMRI studies of the infant brain

Table 1c

A summary of the analysis techniques used in all infant functional NIRS studies published since the first study in 1998 (RM: repeated measure, FDR: false discovery rate, algorithm: automatic detection of artifacts, video: visual inspection of infant movement, visual: visual inspection of data).

	First author	Year	Statistical methods	Image reconstruction	Baseline correction	Treatment of artifacts
1	Meek	1998	Average change (<i>t</i> -test)	No	n/r	Algorithm
2	Sakatani	1999	Average change (<i>t</i> -test)	No	n/r	n/r
3	Hoshi	2000	Average change (<i>t</i> -test)	No	n/r	No
4	Bartocci	2000	Time course analysis (RM-ANOVA)	No	n/r	No
5	Zaramella	2001	Average change (<i>t</i> -test)	No	n/r	Algorithm
6	Baird	2002	Time course analysis (RM-ANOVA)	No	n/r	Algorithm
7	Pena	2003	Average change (RM-ANOVA + post hoc comparisons)	Yes	Detrend – block	Algorithm
8	Taga	2003b	Time course analysis (RM-ANOVA)	Yes	High-pass-filter (0.002 Hz)	Algorithm
9	Taga	2003a	Time course analysis (RM-ANOVA)	No	Detrend – session	Algorithm
10	Csibra	2004	Average change (<i>t</i> -test)	No	Detrend – session	Video + Visual
11	Kusaka	2004	Average change (Wilcoxon's signed rank test, Mann–Whitney <i>U</i> -test)	Yes	Detrend – block	n/r
12	Kotilahti	2005	Average around peak change (<i>t</i> -test)	No	n/r	Algorithm
13	Wilcox	2005	Average change	No	n/r	Algorithm
14	Shimada	2006	General linear model	Yes	n/r	Video
15	Homae	2006	Average change (<i>t</i> -test)	Yes	Detrend – block	Algorithm
16	Homae	2007	Average change (<i>t</i> -test)	Yes	Detrend – block	Algorithm
17	Saito	2007a	Average change (<i>t</i> -test)	No	Detrend – block	Algorithm
18	Blasi	2007	Peak change (<i>t</i> -test)	Yes	Detrend – block	Algorithm
19	Bortfield	2007	Average change (ANOVA, <i>t</i> -test)	No	n/r	Algorithm
20	Minagawa-Kawai	2007	Peak change (<i>t</i> -test + Holm correction)	No	n/r	Visual
21	Otsuka	2007	Average change (<i>t</i> -test); Time course analysis (RM-ANOVA)	No	High-pass-filter (0.02 Hz)	Video + Algorithm
22	Saito	2007b	Average change (ANOVA)	Yes	Detrend – session	Algorithm
23	Taga	2007	Average change (<i>t</i> -test + FDR correction)	No	Detrend – block	Visual
24	Taga	2007	Time course analysis (<i>F</i> -test); Average change (<i>t</i> -test, RM-ANOVA)	No	Detrend – block	Video + Algorithm
25	Carlsson	2008	Average change (ANOVA)	No	Detrend – session	Video
26	Karen	2008	Average change (paired Wilcoxon sign rank test)	Yes	Detrend – block low-pass-filter (0.25 Hz)	n/r
27	Wilcox	2008	Average change (<i>t</i> -test, ANOVA)	No	Detrend – block	Algorithm
28	Grossmann	2008	Peak change (<i>t</i> -test + FDR correction)	No	Detrend – block	Algorithm
29	Gervain	2008	Average change (<i>t</i> -test, ANOVA)	No	n/r	n/r
30	Watanabe	2008	Average change (<i>t</i> -test + FDR correction)	No	Detrend – block	Video + Algorithm
31	Nakato	2009	Average change (Z-score, ANOVA)	No	High-pass-filter (0.02 Hz)	Video + Algorithm
32	Nakano	2009	Average change (<i>t</i> -test, ANOVA + FDR correction)	No	Detrend – block	Video + Algorithm
33	Minagawa-Kawai	2009	Average change (<i>t</i> -test + Bonferroni correction)	No	n/r	Video + Visual
34	Wilcox	2009	Average change (<i>t</i> -test, ANOVA)	No	Detrend – block	Algorithm
35	Lloyd-Fox	2009	Peak change (<i>t</i> -test)	No	Detrend – block	Algorithm
36	Bortfeld	2009	Average change (ANOVA)	No	n/r	Video + Algorithm

have also found marked differences in the haemodynamic response to neuronal activation compared to that in the adult brain. The reason for this is not entirely clear although it has been hypothesised that an excess of superfluous synaptic connections in younger infants may play a role (Marcar et al., 2004).

In addition, brain maturation is not homogeneous throughout the brain, which may explain why some researchers have reported that different types of haemodynamic responses have been observed across different regions (Dehaene-Lambertz et al., 2006). In an object processing study by Wilcox et al. (2009), a differential change in HbO₂ concentration across regions, specific to a single experimental condition, was observed. Whereas the featural difference condition produced HbO₂ increases in both the temporal and occipital area, the spatiotemporal-discontinuity condition produced an increase in HbO₂ in the occipital area, and a decrease in HbO₂ in the temporal area. The authors suggested that this unpredicted decrease in HbO₂ could have occurred because the channel covered an inactive area and so the blood supply was redirected to neighbouring active areas of the cortex.

Further understanding of the infant haemodynamic response could come from infant physiological models of brain circulation and metabolism in accord with those proposed for adults (Banaji et al., 2008; Mintun et al., 2001). In addition, simultaneous data acquisition with NIRS and fMRI could provide structural localization of the origin of the signal changes observed in infants. For the present, it is paramount that researchers report both HbO₂ and

HHb changes in infant studies until the relative functional importance of the two chromophores and the inconsistent HbH changes observed in infants can be explored further.

7. Coregistration

One of the main difficulties of NIRS data interpretation is localizing the origin of the haemodynamic response. NIRS measurements are made from the surface of the scalp making it difficult to establish the exact spatial origin within the brain, of the haemodynamic response. In NIRS and EEG studies it is standard practise to use the 10/20 system (Jasper, 1958) to localize regions of interest using external landmarks, but this method does not inform the internal organization of the brain. Hence, NIRS can benefit greatly from the accurate structural cerebral information provided by brain imaging techniques such as MRI. Multimodal data acquisition could contribute crucial information about rapid brain development and changes in head shape and size in the early growth stages.

fMRI and fNIRS view the same physiological phenomenon (the haemodynamic response to neural activation) but measure it using different physical principles with different spatial, temporal and quantitative scales. This has been exploited to enhance the information provided by each technique. For example, the high temporal resolution in fNIRS has been used to explore the transients in the fMRI-BOLD, and the quantitative HbO₂ and

HHb fNIRS signals have been used to investigate the physiological origin of the fMRI-BOLD signal in adults (Steinbrink et al., 2006). More recently, Huppert et al. (2008) have used multimodality fMRI-fNIRS fusion imaging not only to improve the accuracy of the spatial localization of the HbO₂ and HHb changes, but also to provide calibration measurements of the BOLD signal (the percentage of BOLD signal change per micromolar change in deoxy-haemoglobin-measured by a 3 T MRI scanner). This offers the possibility of comparing quantitative changes across participants.

At present, fMRI-fNIRS studies in humans have only been performed in adults (for a review, see Steinbrink et al., 2006). Nevertheless, it would be of great interest to use this multimodal approach to more fully characterize the haemodynamic response in the developing brain. One of the primary objectives of such studies would be to investigate whether the conflicting adult and infant haemodynamic responses to similar stimuli are a result of the stimulation protocol, the measurement systems, or differences in neurovascular coupling related physiology. Moreover, it could be beneficial to combine Diffusion Tensor Imaging (DTI) (infant myelination has also been investigated using spin labeled perfusion MRI; Wang et al., 2008, and T1 and T2 measurements; Sano et al., 2007) with NIRS for the study of myelination in infants. As the infants are usually asleep when they have a myelination scan such as DTI, integrating fNIRS would be limited to the study of auditory or stroboscopic light stimuli. The rationale for using these techniques in parallel is the same as that for combining fMRI and DTI. Multimodality integration studies of brain connectivity can enhance our understanding of structure–function relationships (Rykhlevskaia et al., 2008). This knowledge can then be applied to clinical investigation of relationships between structural brain damage and functional connections and subsequent impairment (Seghier et al., 2004). Further, fMRI and fNIRS can assist DTI by focusing on the anatomical connections to a localized region of interest, substantially reducing data collection and computational resources, which are very high in fibre tracking procedures.

A final multimodality integration technique that will enhance our understanding of infant brain development is combined NIRS-EEG research. Though neither of these will inform the underlying structural anatomy they can provide complimentary functional information of the spatial and temporal localization of the signal. A study by Grossmann et al. (2008) used each technique to investigate social perception of eye gaze in two groups of infants. They found correlation between the spatial response measured by NIRS and by EEG and further, using the temporal information from the EEG recordings, they were able to deconvolve responses to different components of the social stimuli, which would not have been possible from NIRS measurements alone. Work is underway to provide a method of measuring NIRS and EEG simultaneously in infants to enhance this powerful method of functional investigation similar to that developed for combined NIRS-EEG research in adults (Cooper et al., in press; Moosmann et al., 2003).

In summary, coregistration could lead to better and more accurate interpretation of the information provided by brain imaging techniques. This could be used to define normal cognitive developmental milestones of the infant brain. Detection of abnormal developmental patterns could then lead to early diagnosis of behavioural and cognitive disorders with the option to inform, design and test intervention strategies.

8. Concluding remarks

As has clearly been shown in this review, developmental neuroscience researchers are now readily using fNIRS to measure haemodynamic responses to a range of experimental stimuli. Each

successive year the field widens to include research on object processing, social communication, action observation, face processing and biological motion processing. The capacity of fNIRS for localizing cortical regions of activation and for allowing movement of participants defines its status as one of the most promising neurodevelopment imaging techniques to appear over the last decade. Recent findings reflect this advantage, for example with cortical responses to biological motion processing vs. mechanical motion processing localized in the posterior superior temporal region (Lloyd-Fox et al., 2009) and processing of a mother's face vs. a strangers face localized in the right fronto-temporal region (Carlsson et al., 2008). A promising future for this technique includes the longitudinal investigation of spatially localized developmental changes in brain function. One such study used fNIRS to investigate the development of a language-specific phonemic contrast in infants from the age of 3 months to 28 months (Minagawa-Kawai et al., 2007), finding age-specific onset in varying regions of the cortex. This work will be further enhanced in the future by combined NIRS and MRI studies. Moreover, due to the ease with which this technique can be used with infants and young children (Wartenburger et al., 2007) and the capability of measurements within individuals, fNIRS is ideally suited for research with atypical populations.

As this field of research continues to rapidly expand, it is paramount that the interpretation of, and subsequent claims arising from, fNIRS data are informed by a clear understanding of the complexities of NIRS measurement systems. Further investigation of the characteristics of the infant haemodynamic response using experimental data, physiological models and multimodal studies is imperative, and relies upon multidisciplinary teams addressing relevant targeted research questions. There have been remarkable accomplishments in infant fNIRS research over the last decade encompassing instrument design, probe development, protocol optimization and data analysis and interpretation. These have set a firm foundation for the continued role of fNIRS as an essential tool for advancing developmental neuroscience research in the future.

Acknowledgements

We would like to thank Gergely Csibra, Kathrin Cohen Kadosh and Marko Nardini for comments on an earlier version of this manuscript. This work was supported by the UK Medical Research Council Component Grant G0400120, and a studentship.

Appendix A

The modified Beer Lambert law relates the change in light attenuation to the change in chromophore concentration, assuming homogeneous light absorption and constant optical scattering effects:

$$\Delta A = \alpha \cdot \Delta c \cdot L \cdot DPF$$

where A is light attenuation, α is the specific absorption coefficient and c is the concentration of chromophore of interest. L is the source-detector separation and DPF is the differential pathlength factor, which is dependent upon the tissue type and wavelength. DPF has been measured in the heads of infants of a range of ages (Duncan et al., 1995). If the tissue is illuminated with two wavelengths (λ_1 and λ_2), simultaneous equations can be constructed:

$$\Delta A^{\lambda_1} = L^{\lambda_1} \cdot DPF(\alpha_{\text{HbO}_2}^{\lambda_1} \Delta c_{\text{HbO}_2} + \alpha_{\text{HHb}}^{\lambda_1} \Delta c_{\text{HHb}})$$

$$\Delta A^{\lambda_2} = L^{\lambda_2} \cdot DPF(\alpha_{\text{HbO}_2}^{\lambda_2} \Delta c_{\text{HbO}_2} + \alpha_{\text{HHb}}^{\lambda_2} \Delta c_{\text{HHb}});$$

allowing for the changes in HbO₂ (Δc_{HbO_2}) and Hb (Δc_{HHb}) concentration to be resolved:

$$\Delta c_{\text{HHb}} = \frac{\alpha_{\text{HbO}_2}^{\lambda_1} (A_{\lambda_2}/L^{\lambda_2}) - \alpha_{\text{HbO}_2}^{\lambda_2} (A_{\lambda_1}/L^{\lambda_1})}{\alpha_{\text{HbO}_2}^{\lambda_1} \alpha_{\text{HHb}}^{\lambda_2} - \alpha_{\text{HbO}_2}^{\lambda_2} \alpha_{\text{HHb}}^{\lambda_1}}$$

$$\Delta c_{\text{HbO}_2} = \frac{\alpha_{\text{HHb}}^{\lambda_1} (A_{\lambda_2}/L^{\lambda_2}) - \alpha_{\text{HHb}}^{\lambda_2} (A_{\lambda_1}/L^{\lambda_1})}{\alpha_{\text{HHb}}^{\lambda_1} \alpha_{\text{HbO}_2}^{\lambda_2} - \alpha_{\text{HHb}}^{\lambda_2} \alpha_{\text{HbO}_2}^{\lambda_1}}$$

References

- Aslin, R., Mehler, J., 2005. Near-infrared spectroscopy for functional studies of brain activity in human infants: promise, prospects, and challenges. *J. Biomed. Opt.* 10, 011009-1-3.
- Baird, A.A., Kagan, J., Gaudette, T., Walz, K.A., Herschlag, N., Boas, D.A., 2002. Frontal lobe activation during object permanence: data from near-infrared spectroscopy. *NeuroImage* 16, 1120–1126.
- Banaji, M., Mallet, A., Elwell, C., Nicholls, P., Cooper, C., 2008. A model of brain circulation and metabolism: NIRS signal changes during physiological challenges. *PLoS Biol.* 4, e1000212, doi:10.1371/journal.pcbi.1000212.
- Bartocci, M., Winberg, J., Ruggiero, J., Carmelina, B., Lena, L., Serra, G., Lagercrantz, H., 2000. Activation of olfactory cortex in newborn infants after odor stimulation: a functional near-infrared spectroscopy study. *Pediatr. Res.* 48, 18–23.
- Benaron, D.A., Hintz, S.R., Villringer, A., Boas, D., Kleinschmidt, A., Frahm, J., Hirth, C., Obrig, H., van Houten, J.C., Kermit, E.L., Cheong, W.F., Stevenson, D.K., 2000. Noninvasive functional imaging of human brain using light. *J. Cereb. Blood Flow Metab.* 20, 469–477.
- Blasi, A., Fox, S., Everdell, N., Volein, A., Tucker, L., Csibra, G., Gibson, A., Hebden, J.C., Johnson, M.H., Elwell, C.E., 2007. Investigation of depth dependent changes in cerebral haemodynamics during face perception in infants. *Phys. Med. Biol.* 52, 6849–6864.
- Blasi, A., Phillips, D., Lloyd-Fox, S., Koh, P.H., Elwell, C.E., in press. Automatic detection of motion artifacts in infant functional optical topography studies. *Adv. Exp. Med. Biol.*
- Boas, D.A., Dale, A.M., Franceschini, M.A., 2004. Diffuse optical imaging of brain activation: approaches to optimizing image sensitivity, resolution, and accuracy. *NeuroImage* 23, S278–S288.
- Boden, S., Obrig, H., Köhncke, C., Benav, H., Koch, P., Steinbrink, J., 2007. The oxygenation response to functional stimulation: is there a physiological meaning to the lag between parameters? *NeuroImage* 36, 100–107.
- Bucher, H.U., Edwards, A.D., Lipp, A.E., Duc, G., 1993. Comparison between near infrared spectroscopy and 133Xenon clearance for estimation of cerebral blood flow in critically ill preterm infants. *Pediatr. Res.* 33, 56–60.
- Carlsson, J., Lagercrantz, H., Olson, L., Printz, G., Bartocci, M., 2008. Activation of the right fronto-temporal cortex during maternal facial recognition in young infants. *Acta Paediatr.* 97, 1221–1225.
- Colier, W.N., Quaresima, V., Oeseburg, B., Ferrari, M., 1999. Human motor-cortex oxygenation changes induced by cyclic coupled movements of hand and foot. *Exp. Brain Res.* 129, 457–461.
- Cooper, R.J., Bhatt, D., Everdell, N.L., Hebden, J.C., in press. A tissue-like, optically turbid and electrically conducting phantom for simultaneous EEG and near-infrared imaging. *Phys. Med. Biol.*
- Csibra, G., Henty, J., Volein, A., Elwell, C., Tucker, L., Meeck, J., Johnson, M.H., 2004. Near infrared spectroscopy reveals neural activation during face perception in infants and adults. *J. Pediatr. Neurol.* 2, 85–89.
- Csibra, G., Tucker, L., Johnson, M.H., 2001. Differential frontal cortex activation before anticipatory and reactive saccades in infants. *Infancy* 2, 159–174.
- Dale, A.M., Halgren, E., 2001. Spatiotemporal mapping of brain activity by integration of multiple imaging modalities. *Curr. Opin. Neurobiol.* 11, 202–208.
- Dehaene-Lambertz, G., Dehaene, S., Hertz-Pannier, L., 2002. Functional neuroimaging of speech perception in infants. *Science* 293, 2013–2015.
- Dehaene-Lambertz, G., Hertz-Pannier, L., Dubois, J., Mériaux, S., Roche, A., Sigman, M., Dehaene, S., 2006. Functional organization of perisylvian activation during presentation of sentences in preverbal infants. *PNAS* 103, 14240–14245.
- Delpy, D.T., Cope, M., 1997. Quantification in tissue near-infrared spectroscopy. *Philos. Trans. R. Soc. Lond. B: Biol. Sci.* 352, 649–659.
- Duncan, A., Meeck, J.H., Clemence, M.E., Elwell, C.E., Tyszczyk, L., Mark Cope, M.T., Delpy, D.T., 1995. Optical pathlength measurements on adult head, calf and forearm and the head of the newborn infant using phase resolved optical spectroscopy. *Phys. Med. Biol.* 40, 295–304.
- Eichele, T., Specht, K., Moosmann, M., Jongsma, M.L.A., Quiroga, R.Q., Nordby, H., Hugdahl, K., 2005. Assessing the spatiotemporal evolution of neuronal activation with single-trial event-related potentials and functional MRI. *PNAS* 102, 17798–17803.
- Elwell, C.E., 1995. A Practical Users Guide to Near Infrared Spectroscopy. Hamamatsu Photonics, UK.
- Elwell, C.E., Springett, R., Hillman, E., Delpy, D.T., 1999. Oscillations in cerebral haemodynamics: implications for functional activation studies. *Adv. Exp. Med. Biol.* 471, 57–65.
- Everdell, N.L., Gibson, A.P., Tullis, I.D.C., Vaithianathan, T., Hebden, J.C., Delpy, D.T., 2005. A frequency multiplexed near-infrared topography system for imaging functional activation in the brain. *Rev. Sci. Instrum.* 76, 093705.
- Ferrari, M., Mottola, L., Quaresima, V., 2004. Principles techniques, and limitations of near infrared spectroscopy. *Can. J. Appl. Physiol.* 29, 463–487.
- Franceschini, M.A., Joseph, D.K., Huppert, T.J., Diamond, S.G., Boas, D., 2006. Diffuse imaging of the whole head. *J. Biomed. Opt.* 11, 054007-1-10.
- Franceschini, M.A., Thaker, S., Themelis, G., Krishnamoorthy, K.K., Bortfeld, H., Diamond, S.G., Boas, D.A., Arvin, K., Grant, P.E., 2007. Assessment of infant brain development with frequency-domain near-infrared spectroscopy. *Pediatr. Res.* 61, 546–551.
- Fukui, Y., Ajichi, Y., Okada, E., 2003. Monte Carlo prediction of near-infrared light propagation in realistic adult and neonatal head models. *Appl. Opt.* 42, 2881–2887.
- Gervain, J., Macagno, F., Cogoi, S., Peña, M., Mehler, J., 2008. The neonate brain detects speech structure. *PNAS* 105, 14222–14227.
- Gibson, A., Hebden, J., Arridge, S., 2005. Recent advances in diffuse optical imaging. *Phys. Med. Biol.* 50, R1–R43.
- Grossmann, T., Johnson, M.H., Lloyd-Fox, S., Blasi, A., Deligianni, F., Elwell, C., Csibra, G., 2008. Early cortical specialization for face-to-face communication in human infants. *Proc. R. Soc. B* 275, 2803–2811.
- Hebden, J.C., 2003. Advances in optical imaging of the newborn infant brain. *Psychophysiology* 40, 501–510.
- Heekeren, H., Kohl, M., Obrig, H., Rudiger, W., Pannwitz, W., Matcher, S., Dirnagl, U., Cooper, C., Villringer, A., 1999. Noninvasive assessment of changes in cytochrome-c oxidase oxidation in human subjects during visual stimulation. *J. Cereb. Blood Flow Metab.* 19, 592–603.
- Hintz, S.R., Benaron, D.A., Siegel, A.M., Zourabian, A., Stevenson, S.K., Bas, D.A., 2001. Bedside functional imaging of the premature infant brain during passive motor activation. *J. Perinat. Med.* 29, 335–343.
- Homae, F., Watanabe, H., Nakano, T., Asakawa, K., Taga, G., 2006. The right hemisphere of sleeping infant perceives sentential prosody. *Neurosci. Res.* 56, 776–780.
- Homae, F., Watanabe, H., Nakano, T., Taga, G., 2007. Prosodic processing in the developing brain. *Neurosci. Res.* 59, 29–39.
- Hoshi, Y., Kohri, S., Matsumoto, Y., Kazutoshi, C., Matsuda, T., Okajima, S., Fujimoto, S., 2000. Haemodynamic responses to photic stimulation in neonates. *Pediatr. Neurol.* 23, 323–327.
- Hou, X.L., Zhou, C.L., Huang, L., Ding, H.S., Tang, Z.Z., Jiang, Y., 2006a. Evaluation of early cognitive ability of infants born preterm by near-infrared spectroscopy. *Zhongguo Dang Dai Er Ke Za Zhi.* 8, 361–364.
- Hou, X.L., Zhou, C.L., Huang, L., Ding, H.S., Wang, H.M., 2006b. Evaluation of relationship between early brain response and neurodevelopment in newborns by using near infrared spectroscopy. *Zhonghua Er Ke Za Zhi.* 44, 445–449.
- Huotilainen, M., Kujala, A., Hotakainen, M., Shestakova, A., Kushnerenko, E., Parkkonen, L., Fellman, V., Näätänen, R., 2003. Auditory magnetic responses of healthy newborns. *NeuroReport* 14, 1871–1875.
- Huettel, S.A., Song, A.W., McCarthy, G., 2003. Functional Magnetic Resonance Imaging. Sinaur Associates Inc., Sunderland, MA.
- Huppert, T.J., Diamond, S.G., Boas, D.A., 2008. Direct estimation of evoked hemoglobin changes by multimodality fusion imaging. *J. Biomed. Opt.* 13, 054031.
- Huppert, T.J., Diamond, S.G., Franceschini, M.A., Boas, D.A., 2009. HomER: a review of time-series analysis methods for near-infrared spectroscopy of the brain. *Appl. Opt.* 48, D280–D298.
- Huppert, T.J., Hoge, R.D., Diamond, S.G., Franceschini, M.A., Boas, D.A., 2006. A temporal comparison of BOLD, ASL and NIRS haemodynamic responses to motor stimuli in adult humans. *NeuroImage* 29, 368–382.
- Ijichi, S., Kusaka, T., Isobe, K., Okubo, K., Kawada, K., Namba, M., Okada, H., Nishida, T., Imai, T., Itoh, S., 2005. Developmental changes of optical properties in neonates determined by near-infrared time-resolved spectroscopy. *Pediatr. Res.* 58, 568–573.
- Imada, T., Zhang, Y., Cheour, M., Taulu, S., Ahonen, A., Kuhl, P.K., 2006. Infant speech perception activates Broca's area: a developmental magnetoencephalography study. *Neuroreport* 17, 957–962.
- Jasper, H.H., 1958. Report of the committee on methods of clinical examination in electroencephalography. *Elect. Clin. Neurophysiol.* 10, 370–371.
- Jöbsis, F.F., 1977. Noninvasive, infrared monitoring of cerebral and myocardial oxygen sufficiency and circulatory parameters. *Science* 198, 1264–1267.
- Jöbsis vander-Vleit, F.F., 1999. Discovery of the near-infrared window into the body and the early development of near-infrared spectroscopy. *J. Biomed. Opt.* 4, 392–396.
- Karen, T., Morren, G., Haensse, D., Bauschatz, A.S., Bucher, H.U., Wolf, M., 2008. Hemodynamic response to visual stimulation in newborn infants using functional near-infrared spectroscopy. *Hum. Brain Mapp.* 29, 453–460.
- Katura, T., Tanaka, N., Obata, A., Sato, H., Maki, A., 2006. Quantitative evaluation of interrelations between spontaneous low-frequency oscillations in cerebral hemodynamics and systemic cardiovascular dynamics. *NeuroImage* 31, 1600–1592.
- Kleinschmidt, A., Obrig, H., Requardt, M., Merboldt, K.D., Dirnagl, U., Villringer, A., Frahm, J., 1996. Simultaneous recording of cerebral blood oxygenation changes during human brain activation by magnetic resonance imaging and near-infrared spectroscopy. *J. Cereb. Blood Flow Metab.* 16, 817–826.
- Kocsis, L., Herman, P., Eke, A., 2006. The modified Beer–Lambert law revisited. *Phys. Med. Biol.* 51, N91–N98.
- Koh, P.H., Elwell, C.E., Delpy, D.T., 2009. Development of a dynamic test phantom for optical topography. *Adv. Exp. Med. Biol.* 645, 141–146.
- Koh, P.H., Glaser, D.E., Flandin, G., Kiebel, S., Butterworth, B., Maki, A., Delpy, D.T., Elwell, C.E., 2007. Functional optical signal analysis: a software tool for near-

- infrared spectroscopy data processing incorporating statistical parametric mapping. *J. Biomed. Opt.* 12, 064010-1083-3668.
- Kotilahti, K., Nissailä, I., Huotilainen, M., Makelä, R., Gavrielides, N., Noponen, T., Björkman, P., Fellman, V., Katila, T., 2005. Bilateral hemodynamic responses to auditory stimulation in newborn infants. *Neuroreport* 16, 1373–1377.
- Krekelberg, B., Boynton, G.M., Wezel, R.J.A., 2006. Adaptation: from single cells to BOLD signals. *Trends Neurosci.* 29, 250–256.
- Kusaka, T., Kawada, K., Okubo, K., Nagano, K., Namba, M., Okada, H., Imai, T., Isobe, K., Itoh, S., 2004. Noninvasive optical imaging in the visual cortex in young infants. *Hum. Brain Mapp.* 22, 122–132.
- Lloyd-Fox, S., Blasi, A., Volein, A., Everdell, N., Elwell, C., Johnson, M.H., 2009. Social perception in infancy: a near infrared spectroscopy study. *Child Dev.* 80, 986–999.
- Logothetis, N., 2003. The underpinnings of the BOLD functional magnetic resonance imaging signal. *J. Neurosci.* 23, 3963–3971.
- Luck, S.J., 2005. *An Introduction to the Event-related Potential Technique*. MIT Press, Cambridge, MA.
- Marcar, V.L., Strassle, A.E., Loenneker, T., Schwarz, U., Martin, E., 2004. The influence of cortical maturation on the BOLD response: an fMRI study of visual cortex in children. *Pediatr. Res.* 56, 967–974.
- Marcar, V.L., Schwarz, U., Martin, E., Loenneker, T., 2006. How depth of anesthesia influences the blood oxygenation level-dependent signal from the visual cortex of children. *Am. J. Neuroradiol.* 27, 799–805.
- Martin, E., Jocri, P., Loenneker, T., Ekatothramis, D., Vitacco, D., Hennig, J., Marcar, V.L., 1999. Visual processing in infants and children studied using functional MRI. *Pediatr. Res.* 46, 135–140.
- Matthews, F., Pearlmuter, B.A., Ward, T.E., Soraghan, C., Markham, C., 2008. Hemodynamics for brain-computer interfaces (optical correlates of control signals). *IEEE Signal Process. Mag.* 25, 87–94.
- Meek, J., 2002. Basic principles of optical imaging and application to the study of infant development. *Dev. Sci.* 5, 371–380.
- Meek, J.H., Firbank, M., Elwell, C.E., Atkinson, J., Braddick, O., Wyatt, J.S., 1998. Regional haemodynamic responses to visual stimulation in awake infants. *Pediatr. Res.* 43, 840–843.
- Minagawa-Kawai, Y., Matsuoka, S., Dan, I., Naoi, N., Nakamura, K., Kojima, S., 2009. Prefrontal activation associated with social attachment: facial-emotion recognition in mothers and infants. *Cereb. Cortex* 19, 284–292.
- Minagawa-Kawai, Y., Mori, K., Naoi, N., Kojima, S., 2007. Neural attunement processes in infants during the acquisition of a language-specific phonemic contrast. *J. Neurosci.* 27, 315–321.
- Minagawa-Kawai, Y., Mori, K., Hebden, J.C., Dupoux, E., 2008. Optical imaging of infants' neurocognitive development: recent advances and perspectives. *Dev. Neurobiol.* 68, 712–728.
- Mintun, M.A., Lundstrom, B.N., Snyder, A.Z., Vlassenko, A.G., Schulman, G.L., Raichle, M.E., 2001. Blood flow and oxygen delivery to human brain during functional activity: theoretical modeling and experimental data. *Proc. Natl. Acad. Sci. U.S.A.* 98, 6859–6864.
- Moosmann, M., Ritter, R., Krastel, I., Brink, A., Thees, S., Blankenburg, F., Taskina, B., Obrig, H., Villringer, A., 2003. Correlates of alpha rhythm in functional magnetic resonance imaging and near infrared spectroscopy. *Neuroimage* 20, 145–158.
- Nakano, T., Watanabe, H., Homae, F., Taga, G., 2009. Prefrontal cortical involvement in young infants' analysis of novelty. *Cereb. Cortex* 19, 455–463.
- Nakato, E., Otsuka, Y., Kanazawa, S., Yamaguchi, M.K., Watanabe, S., Kakigi, R., 2009. When do infants differentiate profile face from frontal face? A near-infrared spectroscopic study. *Hum. Brain Mapp.* 30, 462–472.
- Nicklin, S., Hassan, I., Wickramasinghe, Y., Spencer, S., 2003. The light still shines, but not that brightly? The current status of perinatal near infrared spectroscopy. *Arch. Dis. Child Fetal Neonatal.* 88, F263–F268.
- Obrig, H., Villringer, A., 2003. Beyond the visible—imaging the human brain with light. *J. Cereb. Blood Flow Met.* 23, 1–8.
- Obrig, H., Neufang, M., Wenzel, R., Kohl, M., Steinbrink, J., Einhaupl, K., Villringer, A., 2000. Spontaneous low frequency oscillations of cerebral hemodynamics and metabolism in human adults. *NeuroImage* 12, 639–623.
- Okada, E., Firbank, M., Schweiger, M., Arridge, S.R., Cope, M., Delpy, D.T., 1997. Theoretical and experimental investigation of near-infrared light propagation in a model of the adult head. *Appl. Opt.* 36, 21–31.
- Otsuka, Y., Nakato, E., Kanazawa, S., Yamaguchi, M.Y., Watanabe, S., Kakigi, R., 2007. Neural activation to upright and inverted faces in infants measured by near infrared spectroscopy. *NeuroImage* 34, 399–406.
- Peña, M., Maki, A., Kovacic, D., Dehaene-Lambertz, G., Koizumi, H., Bouquet, F., Mehler, J., 2003. Sounds and silence: an optical topography study of language recognition at birth. *PNAS* 100, 11702–11705.
- Raichle, M.E., 1998. Behind the scenes of functional brain imaging: a historical and physiological perspective. *PNAS* 95, 765–772.
- Rykhlevskaia, E., Gratton, G., Fabiani, M., 2008. Combining structural and functional neuroimaging data for studying brain connectivity: a review. *Psychophysiology* 45, 173–187.
- Saager, R., Berger, A., 2008. Measurement of layer-like hemodynamic trends in scalp and cortex: implications for physiological baseline suppression in functional near-infrared spectroscopy. *J. Biomed. Opt.* 13, 034017.
- Saito, Y., Aoyama, S., Kondo, T., Fukumoto, R., Konishi, N., Nakamura, K., Kobayashi, M., Toshima, T., 2007a. Frontal cerebral blood flow change associated with infant-directed speech. *Arch. Dis. Child.* 92, F113–F116.
- Saito, Y., Kondo, T., Aoyama, S., Fukumoto, R., Konishi, N., Nakamura, K., Kobayashi, M., Toshima, T., 2007b. The function of the frontal lobe in neonates for response to a prosodic voice. *Early Hum. Dev.* 83, 225–230.
- Sakatani, K., Chen, S., Lichty, W., Zuo, H., Wang, Y., 1999. Cerebral blood oxygenation changes induced by auditory stimulation in newborn infants measured by near infrared spectroscopy. *Early Hum. Dev.* 55, 229–236.
- Sakatani, K., Yamashita, D., Yamanaka, T., Oda, M., Yamashita, Y., Hoshino, T., Fujiwara, N., Murata, Y., Katayama, Y., 2006. Changes of cerebral blood oxygenation and optical pathlength during activation and deactivation in the prefrontal cortex measured by time-resolved near infrared spectroscopy. *Life Sci.* 78, 2734–2741.
- Salamon, G., Raynaud, C., Regis, J., Rumeau, C., 1990. *Magnetic Resonance Imaging of the Pediatric Brain*. Raven Press, New York.
- Sano, M., Kaga, K., Kuan, C.-C., Ino, K., Mima, K., 2007. Early myelination patterns in the brainstem auditory nuclei and pathway: MRI evaluation study. *Int. J. Ped. Otorhinol.* 71, 1105–1115.
- Sato, H., Kiguchi, M., Kawaguchi, F., Maki, A., 2004. Practicality of wavelength selection to improve signal-to-noise ratio in infrared spectroscopy. *NeuroImage* 21, 1554–1562.
- Schroeter, M.L., Bücheler, M.M., Müller, K., Uludag, K., Obrig, H., Lohmann, G., Tittgemeyer, M., Villringer, A., Cramon, D.Y., 2004. Towards a standard analysis for functional near-infrared imaging. *NeuroImage* 21, 283–290.
- Seghier, M.L., Lazeyras, F., Zimine, S., Maier, S.E., Hanquinet, S., Delavelle, J., Volpe, J.J., Huppi, P.S., 2004. Combination of event-related fMRI and diffusion tensor imaging in an infant with perinatal stroke. *NeuroImage* 21, 463–472.
- Shimada, S., Hiraki, K., 2006. Infant's brain responses to live and televised action. *NeuroImage* 32, 930–939.
- Siegel, A., Marota, J.J., Boas, D., 1999. Design and evaluation of a continuous-wave diffuse optical tomography system. *Opt. Express* 4, 287–298.
- Singh, A.K., Dan, I., 2006. Exploring the false discovery rate in multichannel NIRS. *NeuroImage* 33, 542–549.
- Steinbrink, J., Villringer, A., Kempf, F., Haux, D., Boden, S., Obrig, H., 2006. Illuminating the BOLD signal: combined fMRI-fNIRS studies. *Magn. Reson. Imag.* 24, 495–505.
- Strangman, G., Culver, J.P., Thompson, J.H., Boas, D.B., 2002. A quantitative comparison of simultaneous BOLD fMRI and NIRS recordings during functional brain activation. *NeuroImage* 17, 719–731.
- Strangman, G., Franchesini, M.A., Boas, D., 2003. Factors affecting the accuracy of near-infrared spectroscopy concentration calculations for focal changes in oxygenation parameters. *NeuroImage* 18, 865–879.
- Tachtsidis, I., Leung, T.S., Devoto, L., Delpy, D.T., Elwell, C.E., 2008. Measurement of frontal lobe functional activation and related systemic effects: a near-infrared spectroscopy investigation. *Adv. Exp. Med. Biol.* 614, 397–403.
- Taga, G., Asakawa, K., Hirasawa, K., Konishi, Y., 2003a. Haemodynamic responses to visual stimulation in occipital and frontal cortex of newborn infants: a near-infrared optical topography study. *Early Hum. Dev.* 75, S203–S210.
- Taga, G., Asakawa, K., Maki, A., Konishi, Y., Koizumi, H., 2003b. Optical imaging in awake infants by near-infrared optical topography. *PNAS* 100, 10722–10727.
- Taga, G., Asakawa, K., 2007. Selectivity and localization of cortical response to auditory and visual stimulation in awake infants aged 2 to 4 months. *NeuroImage* 36, 1246–1252.
- Taga, G., Homae, F., Watanabe, H., 2007. Effects of source-detector distance of near infrared spectroscopy on the measurement of the cortical hemodynamic response in infants. *NeuroImage* 38, 452–460.
- Taga, G., Konishi, Y., Maki, A., Tachibana, T., Fujiwara, M., Koizumi, H., 2000. Spontaneous oscillation of oxy- and deoxy-haemoglobin changes with a phase difference throughout the occipital cortex of newborn infants observed using non-invasive optical topography. *Neurosci. Lett.* 282, 104–101.
- Toet, M.C., Lemmers, P.M.A., 2009. Brain monitoring in neonates. *Early Hum. Dev.* 85, 77–84.
- Toronov, V., Walker, S., Gupta, R., Choi, J.H., Gratton, E., Hueber, D., Webb, A., 2003. The roles of changes in deoxyhemoglobin concentration and regional cerebral blood volume in the fMRI BOLD signal. *NeuroImage* 19, 1521–1531.
- Tzourio-Mazoyer, N., De Schonen, S., Crivello, F., Reutter, B., Aujard, Y., Mazoyer, B., 2002. Neural correlates of woman face processing by 2-month-old infants. *NeuroImage* 15, 454–461.
- Uludag, K., Steinbrink, J., Villringer, A., Obrig, H., 2004. Separability and cross talk: optimizing dual wavelength combinations for near-infrared spectroscopy of the adult head. *NeuroImage* 22, 583–589.
- Villringer, A., Chance, B., 1997. Noninvasive optical spectroscopy and imaging of human brain function. *Trends Neurosci.* 20, 435–442.
- Walsh, V., Cowey, A., 2000. Transcranial magnetic stimulation and cognitive neuroscience. *Nat Rev Neurosci* 1, 73–79.
- Wang, Z., Fernandez-Seara, M., Aslop, D.C., Liu, W.-C., Flax, J.F., Benasich, A.A., Detre, J.A., 2008. Assessment of functional development in normal infant brain using arterial spin labeled perfusion MRI. *NeuroImage* 39, 973–978.
- Wartenburger, I., Steinbrink, J., Telkemeyer, S., Friedrich, M., Obrig, H., 2007. The processing of prosody: evident of interhemispheric specialization at the age of four. *NeuroImage* 34, 416–425.
- Watanabe, H., Homae, F., Nakano, T., Taga, G., 2008. Functional activation in diverse regions of the developing brain of human infants. *NeuroImage* 43, 346–357.
- Weishaupt, D., Kchli, V.D., Marincek, B., 2008. *How Does MRI Work? An Introduction to the Physics and Function of Magnetic Resonance Imaging*. Springer-Verlag, Berlin Heidelberg.
- Wilcox, T., Bortfeld, H., Woods, R., Wriuck, E., Boas, D.A., 2005. Using near-infrared spectroscopy to assess neural activation during object processing in infants. *J. Biomed. Opt.* 10, 1010–1019.

- Wilcox, T., Bortfeld, H., Woods, R., Wruck, E., Boas, D.A., 2008. Haemodynamic response to featural changes in the occipital and inferior temporal cortex in infants: a preliminary methodological exploration. *Dev. Sci.* 11, 361–370.
- Wilcox, T., Bortfeld, H., Woods, R., Wruck, E., Armstrong, J., Boas, D.A., 2009. Haemodynamic changes in the infant cortex during the processing of featural and spatiotemporal information. *Neuropsychology* 47, 657–662.
- Wolf, M., Ferrari, M., Quaresima, V., 2007. Progress of near-infrared spectroscopy and topography for brain and muscle clinical applications. *J. Biomed. Opt.* 12 062104-1–14.
- Wyatt, J.S., Cope, M., Delpy, D.T., Wray, S., Reynolds, E.O., 1986. Quantification of cerebral oxygenation and haemodynamics in sick newborn infants by near infrared spectrophotometry. *Lancet* 2, 1063–1066.
- Yamashita, Y., Maki, A., Koizumi, H., 2001. Depth dependence of the precision of noninvasive optical measurement of oxy-, deoxy-, and total-hemoglobin concentration. *Med. Phys.* 28, 1108–1114.
- Ye, J.C., Tak, S.H., Jang, K.E., Jung, J.W., Jang, J.D., 2009. NIRS-SPM: statistical parametric mapping for near-infrared spectroscopy. *NeuroImage* 44, 428–447.
- Zaramella, P., Freato, F., Amigoni, A., Salvadori, S., Marangoni, P., Suppiej, A., Schiavo, B., Chiandetti, L., 2001. Brain auditory activation measured by near-infrared spectroscopy (NIRS) in neonates. *Pediatr. Res.* 49, 213–220.
- Zhang, Y., Brooks, D.H., Franceschini, M.A., Boas, D.A., 2005. Eigenvector-based spatial filtering for reduction of physiological interference in diffuse optical imaging. *J. Biomed. Opt.* 10, 011014.